


SciCan BRAVO™ G4 Quick Reference Guide

EUROPEAN UNION +49(0) 7561 98 343-0


Operator's Manual (located on the USB key) should be consulted before using this autoclave.

BASIC OPERATION

1 Power unit ON.

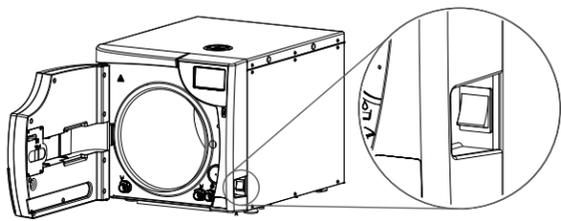


2 Fill with demineralised/distilled water.

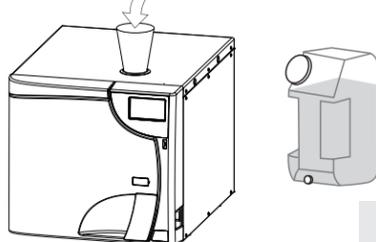


NEVER USE TAP WATER


3 Load configurations.

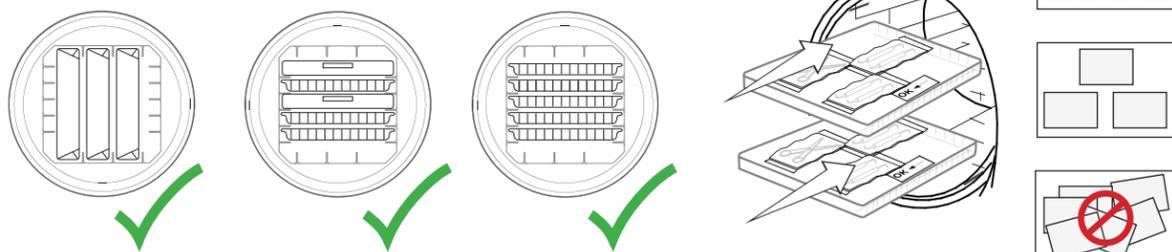


4 Close unit.

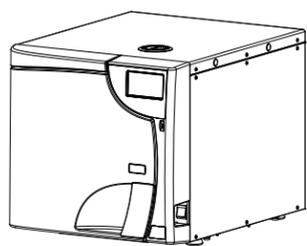


5 Run cycle.

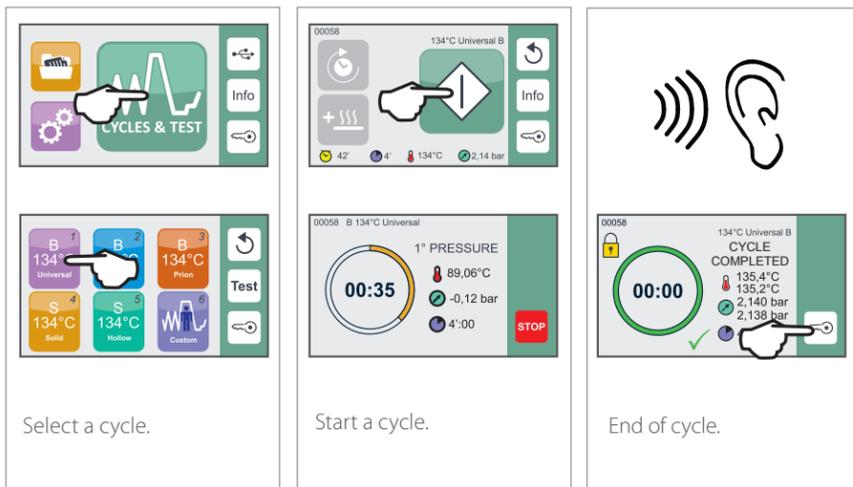


TOUCHSCREEN

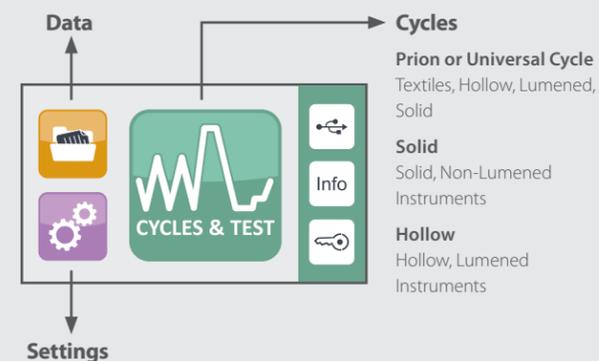


VENTILATION

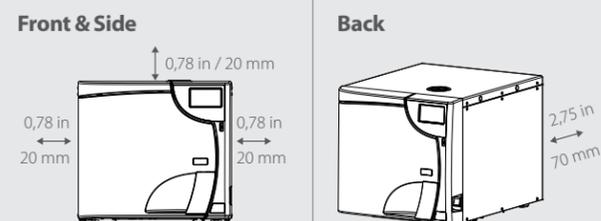


FILLING OPTIONS

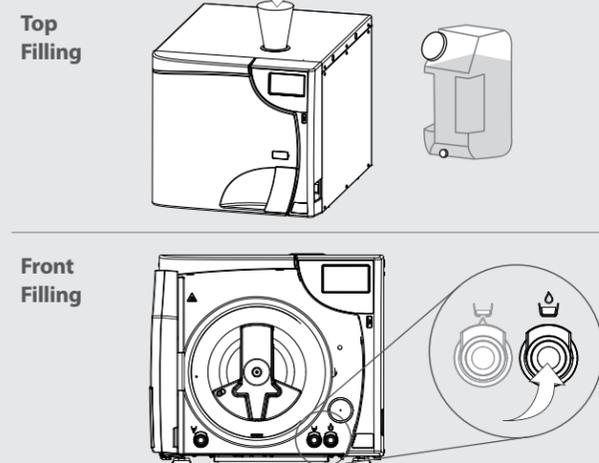


6 Open unit.

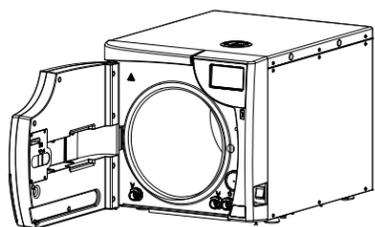


7 Unload instruments.

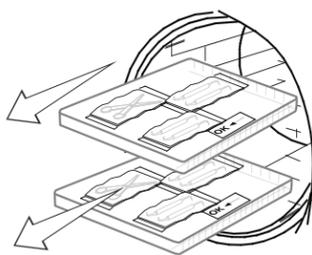

8 If required, drain manually.

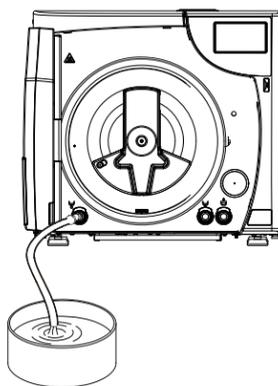

DRAINING OPTIONS

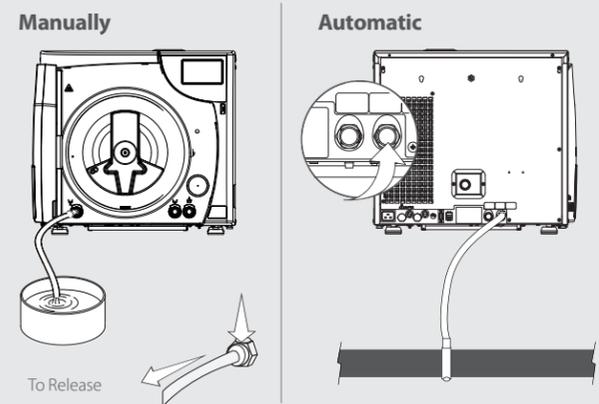

MAINTENANCE SCHEDULE

Daily	Clean the door gasket and internal part of the door with a clean wet cloth. Check for wear and replace if required.	Every 3-6 Months	Check the bacteriological filter and replace as required.
	Completely empty the waste tank before refilling the water reservoir.		Lubricate the door lock . Using a clean cloth, remove any residues and lubricate the inside of the bushing with a film of the silicone-based grease provided.
Weekly	Clean the chamber and appropriate accessories with a wet cloth. If required, use a neutral detergent (without alkalines and bleaches). Carefully rinse with demineralized/distilled water and remove any residue.	Every Year or 1,000 Cycles	Inspect and clean the chamber drain filter .
	Inspect and clean chamber anti-dust filter . Replace if necessary.		Replace if required.
Monthly	Ensure area around BRAVO G4 is dust free.		
	Drain & clean the internal water reservoir as per the instructions outlined in the Operator's Manual.		Replace the door gasket .
	If applicable, clean the external water tank used for automatic filling.		

Spare Parts and Accessories

97400145	Door Gasket 17L/22L
97467176	Door Gasket 28L
97290160	Bacteriological Filter
97290210	Chamber Drain Filter
99950390	Chamber Rack 17L
99950317	Chamber Rack 22L
99951041	Chamber Rack 28L
99950394	Pouch Rack
99951317	Tray 17L
99951318	Tray 22L
99951042	Tray 28L
97467066	Tray Extractor

IMPORTANT!

Users of this device must be sure to select the most appropriate sterilisation cycle according to the recommendations of the leading infection control authorities and local regulatory guidelines / recommendations.